

**THIS PAGE IS INSERTED BY OIPE SCANNING**

**IMAGES WITHIN THIS DOCUMENT ARE BEST AVAILABLE COPY AND CONTAIN DEFECTIVE IMAGES SCANNED FROM ORIGINALS SUBMITTED BY THE APPLICANT.**

**DEFECTIVE IMAGES COULD INCLUDE BUT ARE NOT LIMITED TO:**

**BLACK BORDERS**

**TEXT CUT OFF AT TOP, BOTTOM OR SIDES**

**FADED TEXT**

**ILLEGIBLE TEXT**

**SKEWED/SLANTED IMAGES**

**COLORED PHOTOS**

**BLACK OR VERY BLACK AND WHITE DARK PHOTOS** 

**GRAY SCALE DOCUMENTS**

**IMAGES ARE BEST AVAILABLE COPY.  
RESCANNING DOCUMENTS *WILL NOT*  
CORRECT IMAGES.**

Figure 1

BEST AVAILABLE COPY






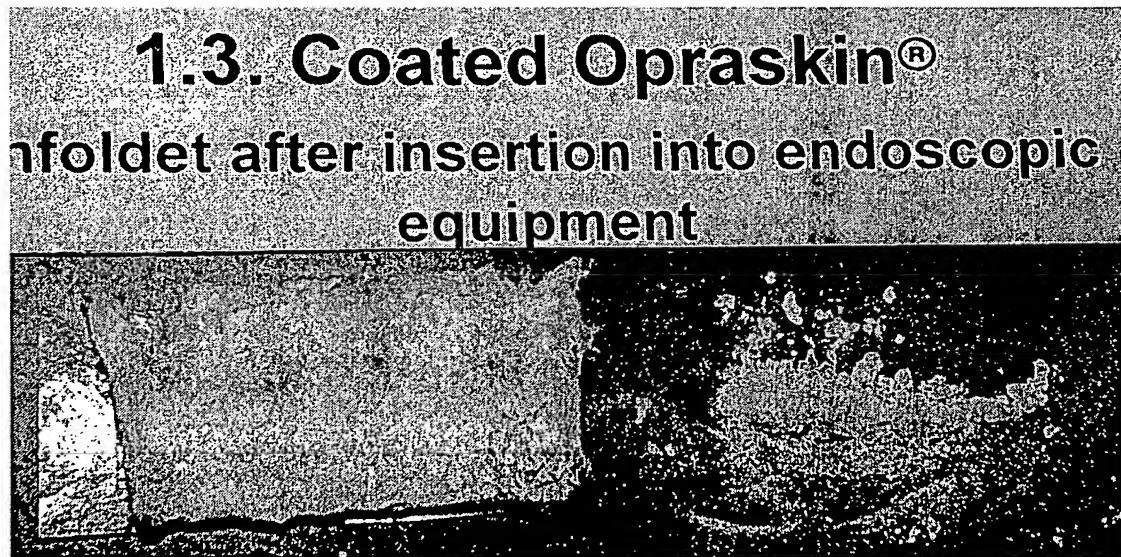


Figure 2

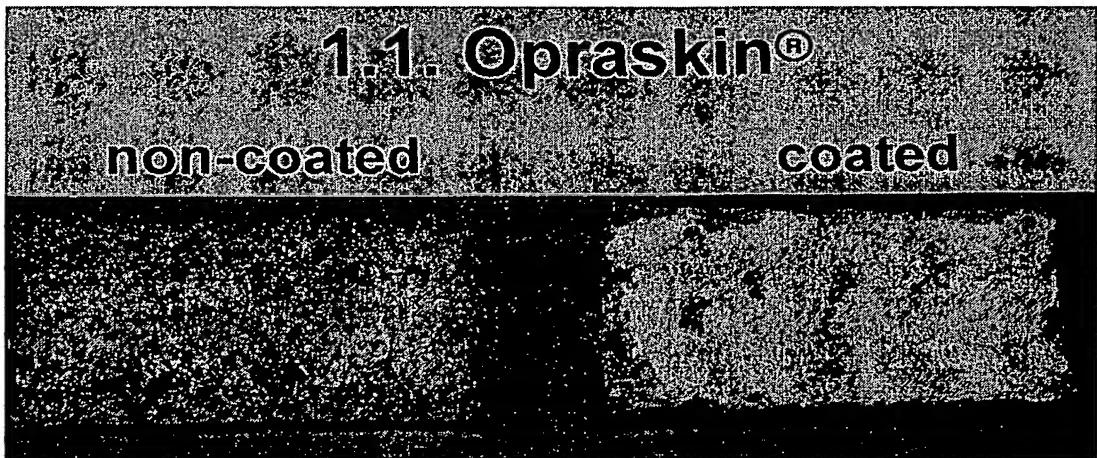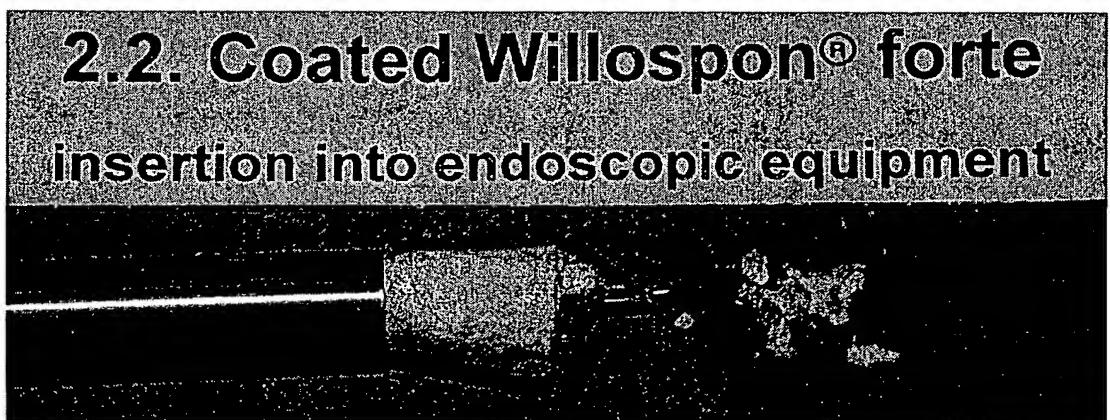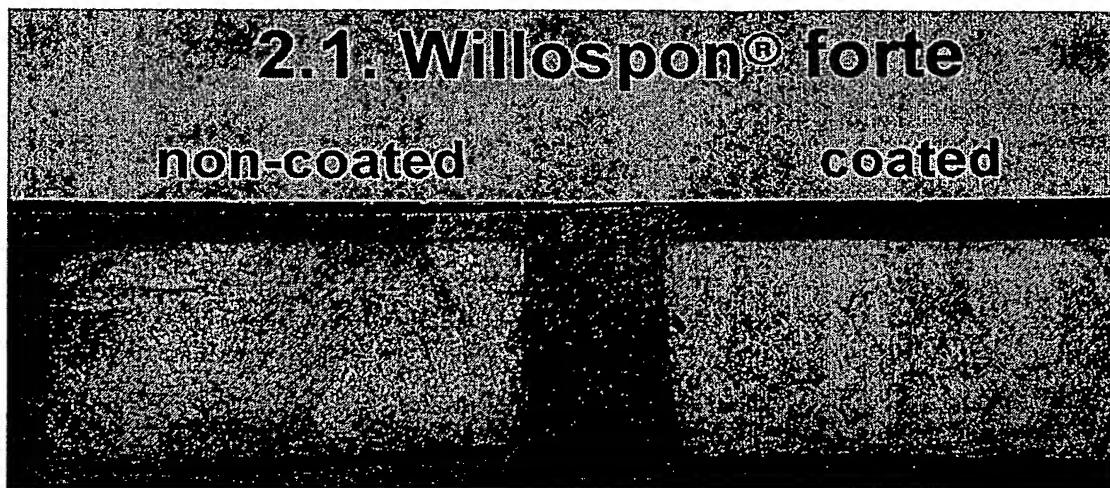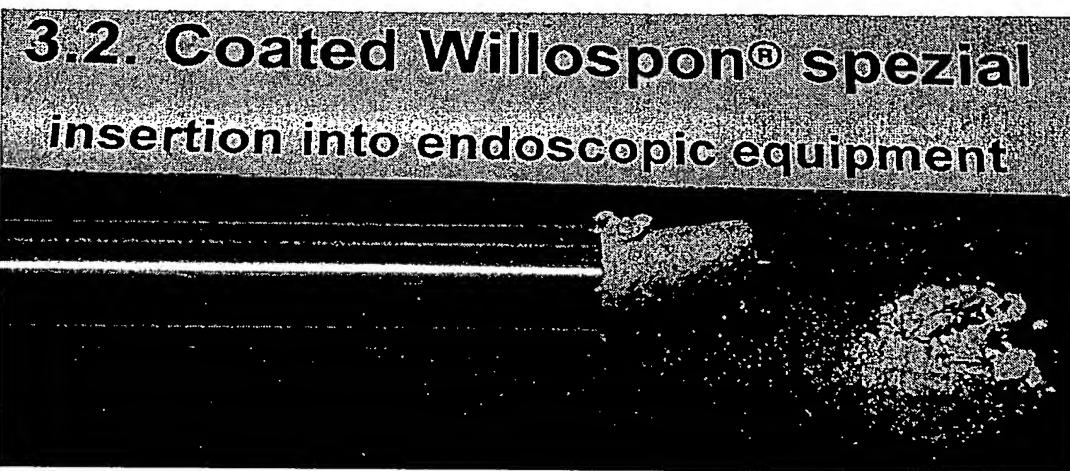

BEST AVAILABLE COPY

Figure 3

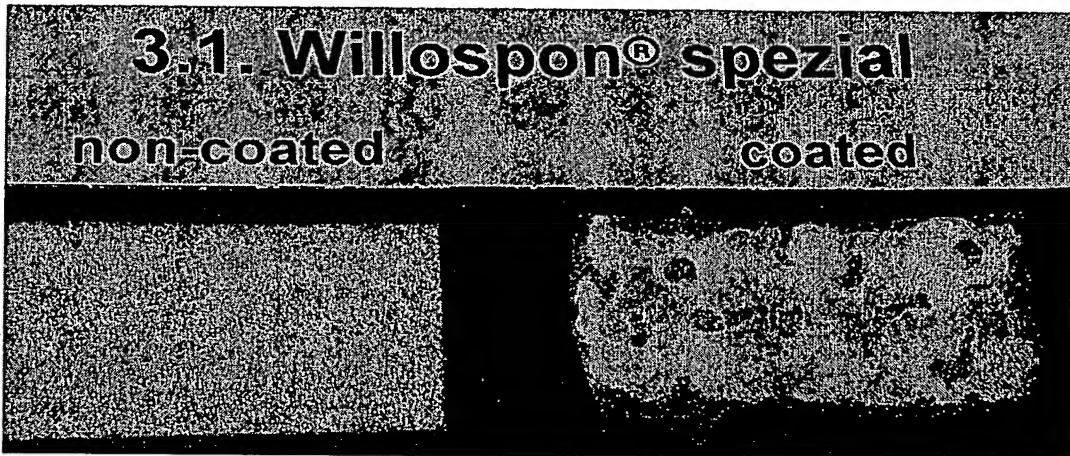


**BEST AVAILABLE COPY**

Figure 4

#### 4.1. Ethisorb® Patch

non-coated

coated

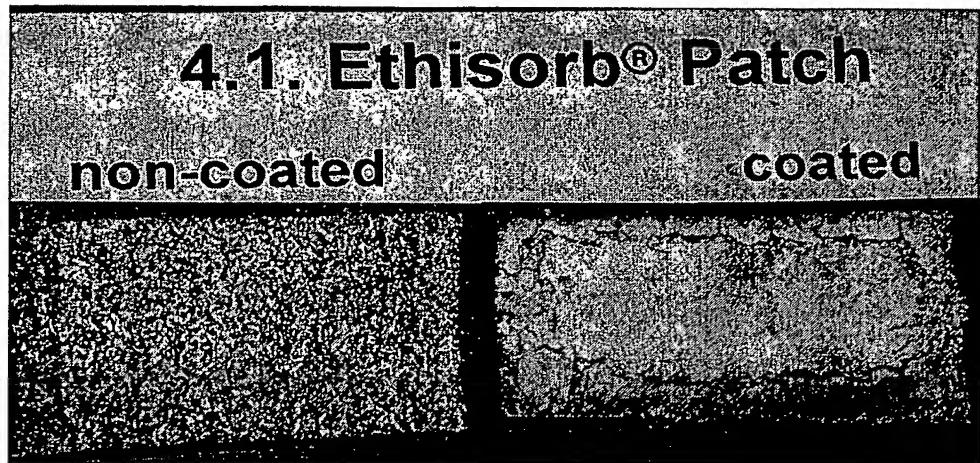


#### 4.2. Coated Ethisorb® Patch

insertion into endoscopic equipment






#### 4.3. Coated Ethisorb® Patch

unfolded after insertion into endoscopic equipment

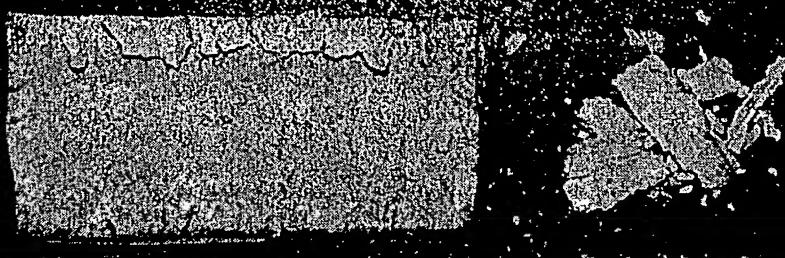



BEST AVAILABLE COPY

Figure 5

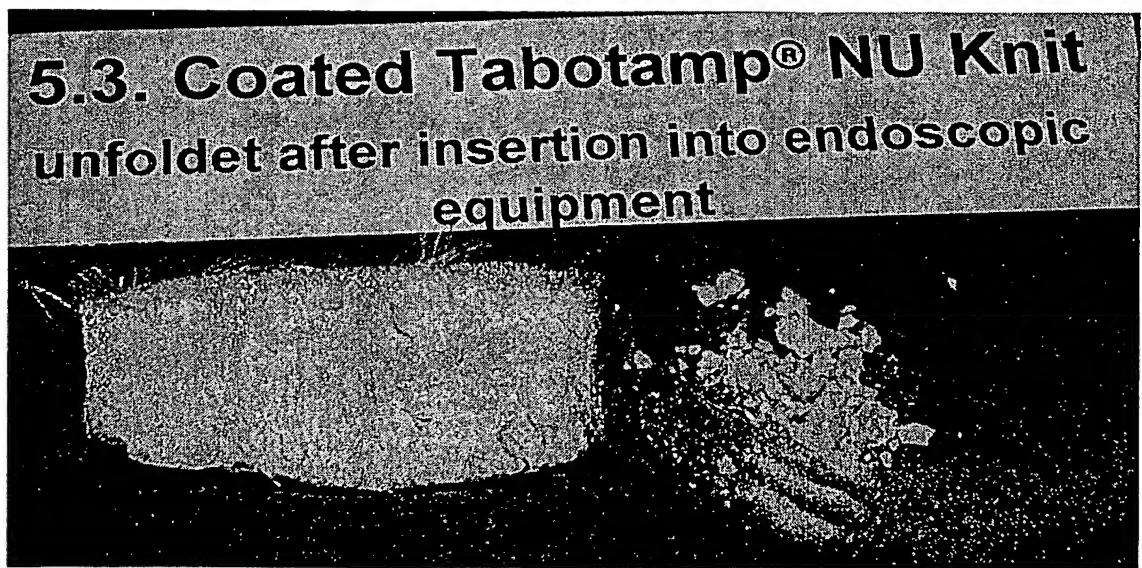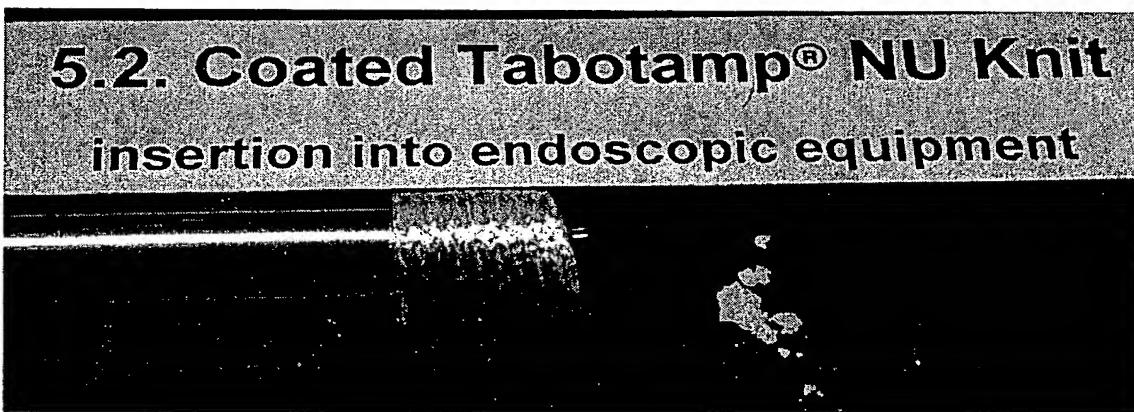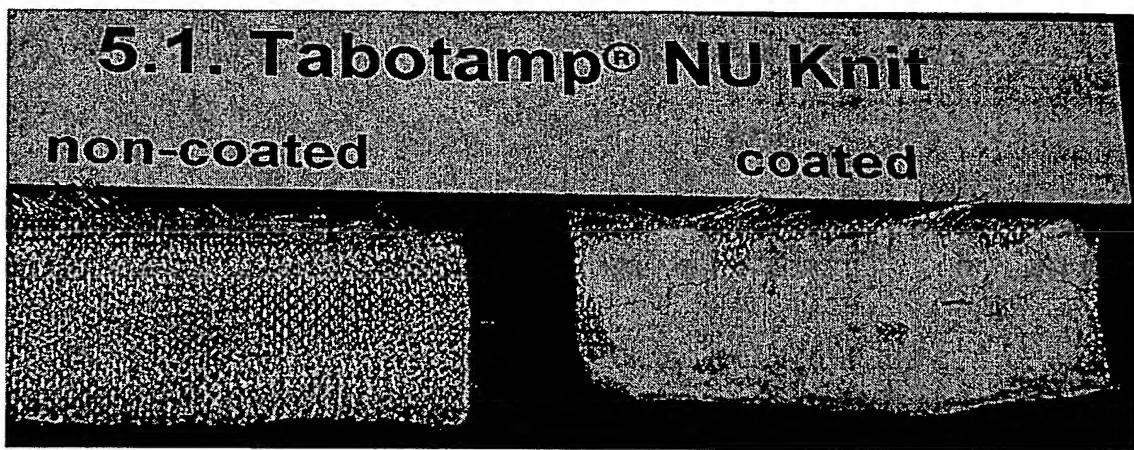

**BEST AVAILABLE COPY**

Figure 7

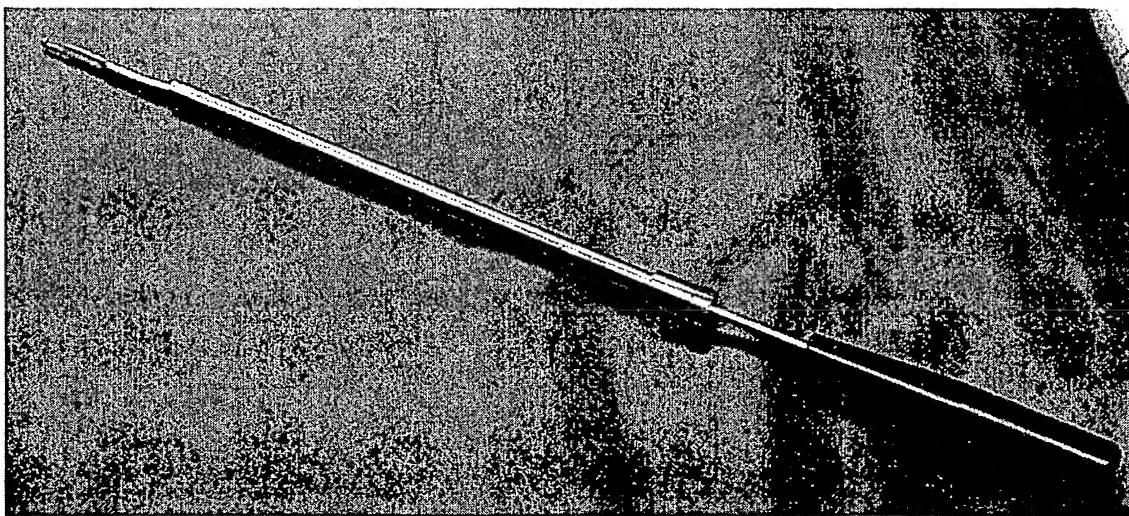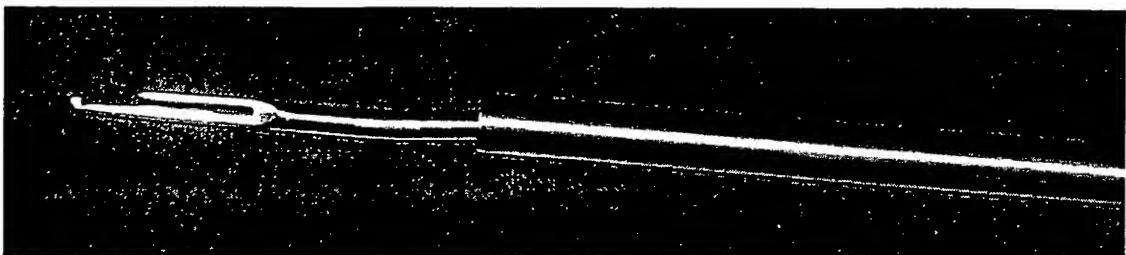

BEST AVAILABLE COPY

Figure 6

## 6.1. Sponge Nycomed

non-coated

coated

## 6.2. Coated Sponge Nycomed

insertion into endoscopic equipment

## 6.3. Coated Sponge Nycomed

unfoldet after insertion into endoscopic equipment


## 6.3. Coated Sponge Nycomed

unfoldet after insertion into endoscopic equipment

Figure 8

Figure 8. Blood coagulation and degradation of clot and carrier patch. The active components of the coating are shown in grey shaded boxes.

5

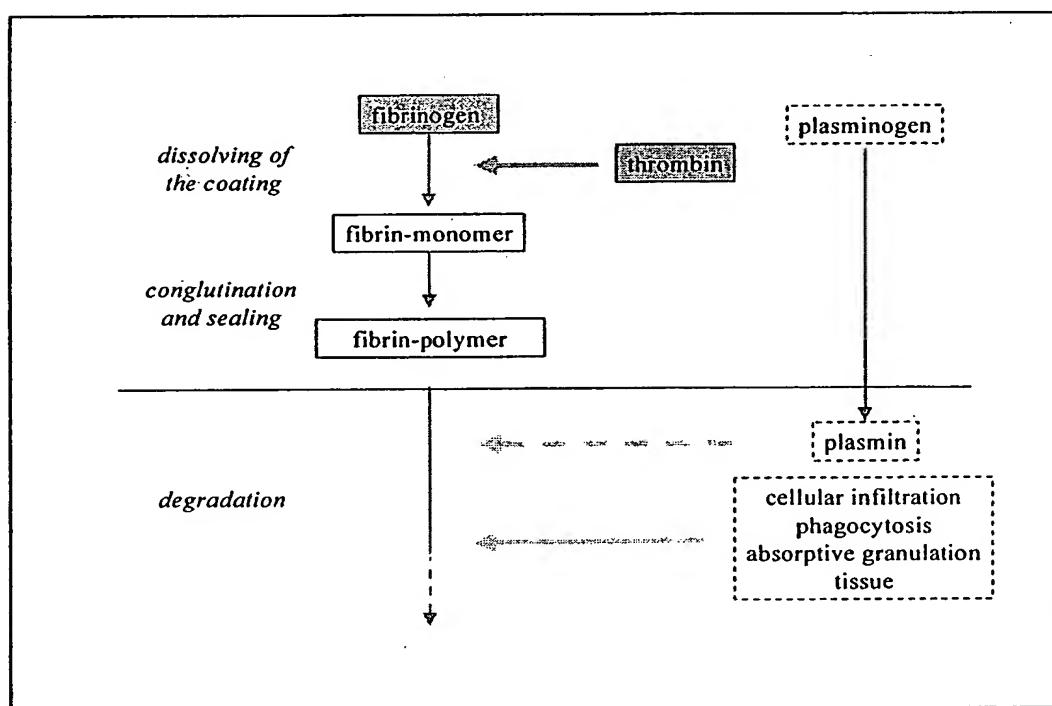

10

BEST AVAILABLE COPY